


Simultaneously and continuously monitors H<sub>2</sub>S, CH<sub>4</sub>, CO<sub>2</sub>, and O<sub>2</sub>

# Biomass gas analyzer <ZPAF>

**Perfect system for your application**

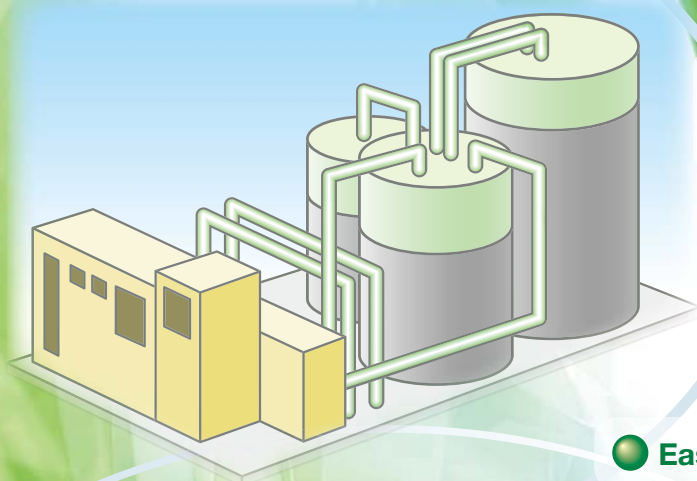

- **Simultaneous and continuous measurement of 4 components: H<sub>2</sub>S, CH<sub>4</sub>, CO<sub>2</sub>, O<sub>2</sub>**


- **Compact and lightweight  
133 × 483 × 382 mm (H×W×D),  
approx. 9 kg**

- **Easy-to-see LCD**

- **A wide variety of optional functions  
Automatic calibration, concentration alarm for upper and lower limit,  
remote input for switching range, range identification signal output, etc.**

# Biomass gasification process

Biogas generated through fermentation of biomass can be used as a fuel for boilers, gas engines, and other applications.

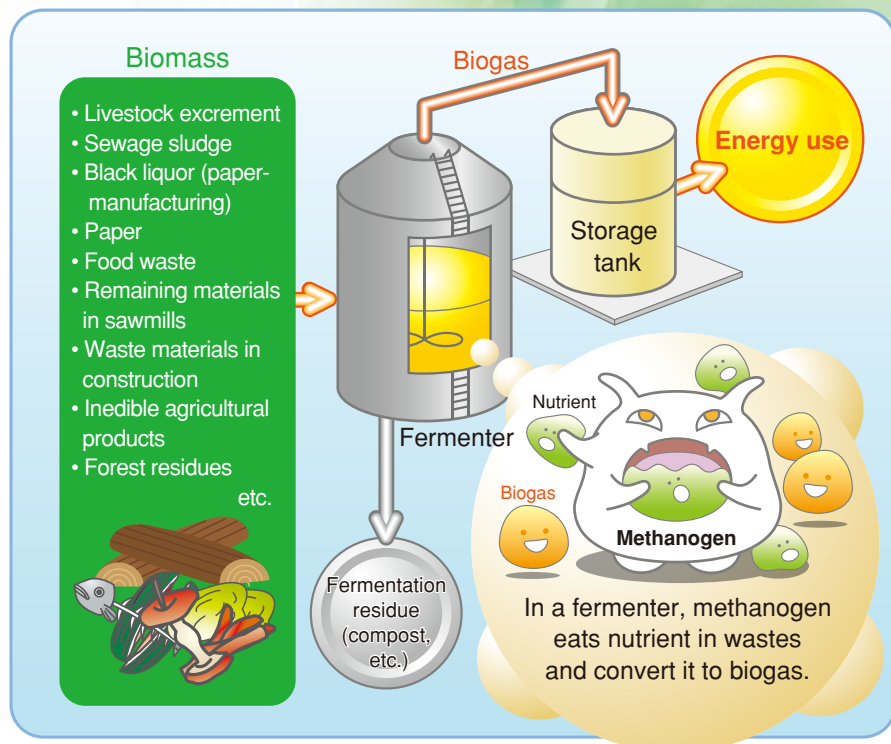

## ● Biogas composition

CH <sub>4</sub>	50 to 75 vol%
CO <sub>2</sub>	25 to 50 vol%
N <sub>2</sub>	0 to 10 vol%
H <sub>2</sub>	0 to 1 vol%
H <sub>2</sub> S	0 to 3 vol%
O <sub>2</sub>	0 to 2 vol%

## ● Biomass resources

- Livestock excrement
- Sewage sludge
- Black liquor (paper - manufacturing)
- Paper
- Food waste
- Remaining materials in sawmills, etc.
- Waste materials in construction
- Inedible agricultural products
- Forest residues

## Features

### Contains 3 sensors necessary for monitoring 4 components


Target gas	Measurement range		Sensor
	1st range	2nd range	
CH <sub>4</sub>	0 to 20 vol%	0 to 100 vol%	Single-beam infrared sensor
CO <sub>2</sub>	0 to 20 vol%	0 to 100 vol%	
H <sub>2</sub> S	0 to 500 ppm	0 to 2000 ppm	Constant-potential electrolytic sensor
O <sub>2</sub>	0 to 10 vol%	0 to 25 vol%	Galvanic cell sensor

### Compact and lightweight



H133 x W483 x D382 mm, approx. 9 kg


### Automatic calibration (optional) eliminates the need for troublesome calibration work

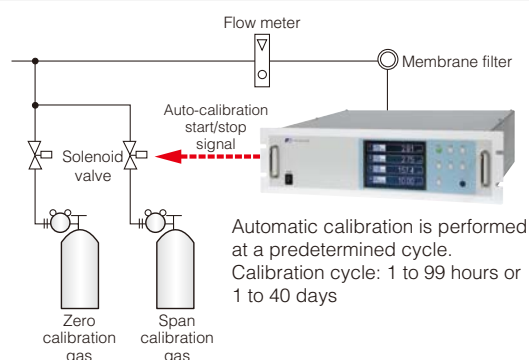

### Gas concentration alarm output (optional)



### RS485 (MODBUS) communication with PC (optional)

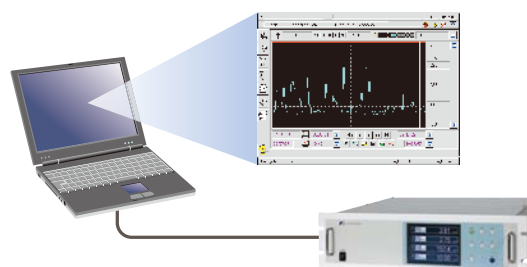

# Specifications

## ■ Main specifications

<b>Principle</b>	CH <sub>4</sub> , CO <sub>2</sub> (Single beam NDIR sensor) O <sub>2</sub> (Galvanic cell sensor) H <sub>2</sub> S (constant-potential electrolytic sensor)		
<b>Display</b>	4-digit backlit LCD		
<b>Components/ range</b>	<b>Component</b>	<b>1st range</b>	<b>2nd range</b>
	CH <sub>4</sub>	0 to 20 vol%	0 to 100 vol%
	CO <sub>2</sub>	0 to 20 vol%	0 to 100 vol%
	H <sub>2</sub> S	0 to 500 ppm	0 to 2000 ppm
	O <sub>2</sub>	0 to 10 vol%	0 to 25 vol%
<b>Number of measurable components</b>	Max. 4 (simultaneous and continuous measurement)		
<b>Analog output</b>	4 to 20 mA DC or 0 to 1 V DC (up to 12 points)		
<b>Contact output (optional)</b>	1c contact (max. 15 points) Device error, calibration error, range identification, auto-calibration status, solenoid valve drive for auto-calibration, limit alarm		
<b>Contact input (optional)</b>	Voltage input (12 to 24 V DC) up to 9 points Remote switchover of ranges, auto-calibration remote start, remote hold		
<b>Output hold</b>	During calibration, output signal can be hold at the value before calibration.		
<b>Range switchover</b>	manual or automatic		
<b>Power supply voltage</b>	100 to 240 V AC, 50/60 Hz		
<b>Power consumption</b>	Approx. 100 VA		
<b>Dimensions</b>	Refer to outline drawing		
<b>Ambient temperature</b>	5°C to 40°C (H <sub>2</sub> S and O <sub>2</sub> sensors: 15°C to 40°C)		
<b>Weight</b>	Approx. 9kg		
<b>Gas inlet/outlet</b>	Rc 1/4 or NPT 1/4 internal thread		
<b>Sensor life expectancy</b>	O <sub>2</sub> sensor: approx. 2 years H <sub>2</sub> S sensor: approx. 1 year		
<b>Certification</b>	CE Marking		

## ■ Performance

<b>Repeatability</b>	±0.5 %FS (H <sub>2</sub> S: ±2.0 %FS)
<b>Linearity</b>	±1 %FS (H <sub>2</sub> S: ±2.0 %FS)
<b>Zero drift</b>	±2 %FS per week
<b>Span drift</b>	±2 %FS (H <sub>2</sub> S: ±2.5 %FS)
<b>Response (90 %FS)</b>	10 to 30 sec. (H <sub>2</sub> S: 120 sec.)
<b>Remote output hold</b>	by external contact input

## ■ Functions

<b>Range identification output</b>	Measurement range can be identified.
<b>Automatic zero/span calibration</b>	can be performed at a predetermined cycle.
<b>Auto-calibration remote start</b>	by external digital input
<b>Simple zero calibration</b>	can be performed at a predetermined cycle.
<b>Upper/lower limit alarm</b>	output when the gas concentration reaches the preset value.
<b>Contact output</b>	· at device error · at calibration error · during auto calibration
<b>Communication</b>	RS485 communication (MODBUS)

## ■ Gas conditions


<b>Flow rate</b>	0.5 ±0.2 L/min
<b>Temperature</b>	10 to 50°C
<b>Pressure</b>	10 kPa or less
<b>Dust</b>	100 µg/Nm <sup>3</sup> or less in particle size of 0.3 µm or smaller

## ■ Replacement sensor


<b>H<sub>2</sub>S sensor</b>	Model: ZP*TQ503691C1
<b>O<sub>2</sub> sensor</b>	Model: ZP*TQ503691C2

# Principle

## ● Constant-potential electrolytic sensor (for H<sub>2</sub>S)

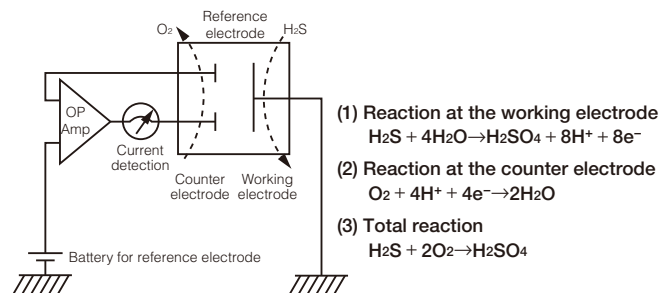


## ● H<sub>2</sub>S measurement

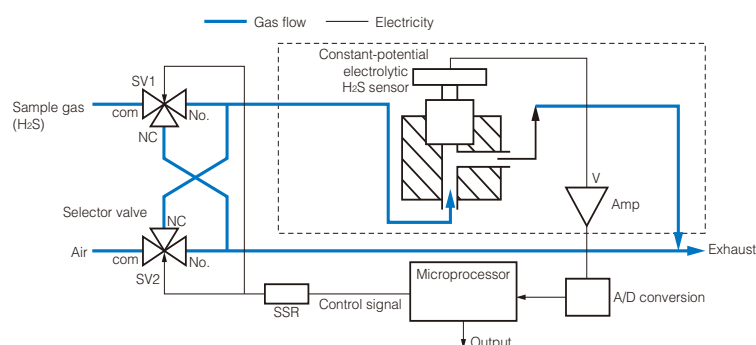


As the H<sub>2</sub>S sensor uses constant-potential electrolytic method, there must be oxygen included in the sample gas. Therefore, air is supplied to the sensor at regular intervals to enable gas analysis in biogas plants where oxygen is absent, and thus stable readings are provided.

## ● Infrared sensor (for CO<sub>2</sub> and CH<sub>4</sub>)

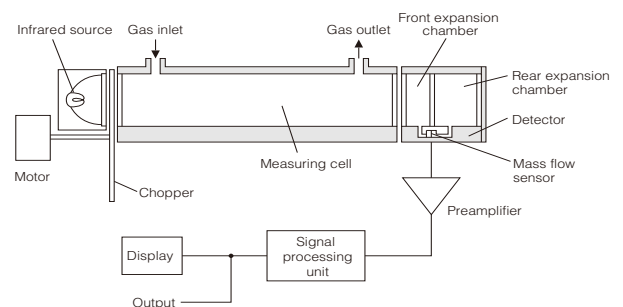

## ● Galvanic fuel cell sensor (for O<sub>2</sub>)

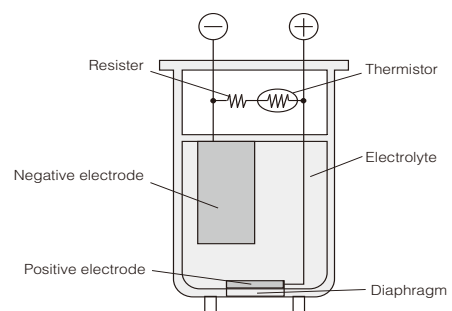

# Model Specifications


4 5 6 7 8 9 10 11 12 13 14 15 16 17 18 19 20 21 22 23 24 25 ← Digit

ZPA FB 1 . Y . YYY . Y YAG

Digit	Specifications	Code
4	Specification	Biomass gas
5	Installation	19-inch rack mount
6	Measured components (CH <sub>4</sub> , CO <sub>2</sub> )	none CO <sub>2</sub> (1st component) CH <sub>4</sub> (1st component) CO <sub>2</sub> (1st component)+CH <sub>4</sub> (2nd component)
7	Measured components (O <sub>2</sub> , H <sub>2</sub> S)	H <sub>2</sub> S O <sub>2</sub> + H <sub>2</sub> S
8	Revision code	1
9	Measurement range (1st component 1st range)	none 0 to 20 vol%
10	Measurement range (1st component 2nd range)	none 0 to 100 vol%
11	Measurement range (2nd component 1st range)	none 0 to 20 vol%
12	Measurement range (2nd component 2nd range)	none 0 to 100 vol%
17	Measurement range (O <sub>2</sub> , H <sub>2</sub> S)	0 to 10/25 vol% O <sub>2</sub> 0 to 500 ppm/2000 ppm H <sub>2</sub> S C+T
18	Gas inlet/outlet size	Rc 1/4 NPT 1/4

Digit	Specifications					Code
19	Output signal	0 to 1 V DC				A
		4 to 20 mA DC				B
		0 to 1 V DC + RS485 communication				C
		4 to 20mA DC + RS485 communication				D
20	Language/Power cable	Japanese/Power cable rated 125 V (PSE)				J
		English/Power cable rated 125 V (UL)				E
		English/Power cable rated 250V (CEE)				U
		Chinese/Power cable rated 250V (CCC)				C
21	-					Y
22	Optional functions (DIO)	FAULT	Auto calibration	Upper/lower limit alarm	Range identification	
		-	-	-	-	Y
		○	-	-	-	A
		○	○	-	-	B
		○	-	○	-	C
		○	-	-	○	D
		○	○	○	-	E
		○	-	○	○	F
		○	○	-	○	G
		○	○	○	○	H
23	-					Y
24	Unit	ppm, vol%				A
25	Adjustment	Biogas				G

## Dimensions (unit: mm)

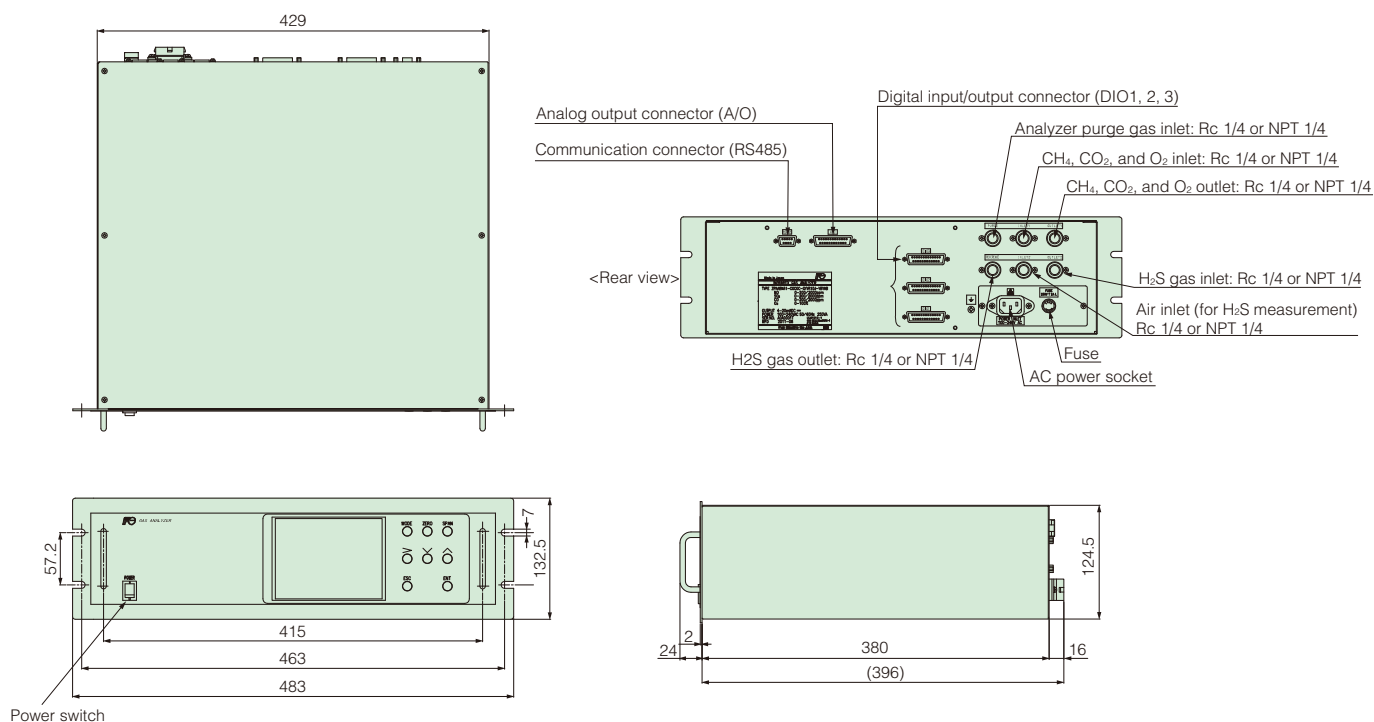

**Fuji Electric Co., Ltd.**

Grobal Sales Section

Instrumentation & Sensors Planning Dept.

1, Fuji-machi, Hino-city, Tokyo 191-8502, Japan

<http://www.fujielectric.com>

Phone: +81-42-514-8930 Fax: +81-42-583-8275

<http://www.fujielectric.com/products/instruments/>